


SC-12-95P



Current Data Parameters  
NAME SC-12-95P  
EXPNO 10  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20221003  
Time 20.04 h  
INSTRUM spect  
PROBHD z116098\_0527 (  
PULPROG zg30  
TD 131072  
SOLVENT CDC13  
NS 16  
DS 0  
SWH 12019.230 Hz  
FIDRES 0.183399 Hz  
AQ 5.4525952 sec  
RG 31.86  
DW 41.600 usec  
DE 11.87 usec  
TE 298.0 K  
D1 0.10000000 sec  
TD0 1  
SFO1 400.2324716 MHz  
NUC1 1H  
P1 10.00 usec  
PLW1 16.02700043 W

F2 - Processing parameters  
SI 131072  
SF 400.2300000 MHz  
WDW EM  
SSB 0  
LB 0.10 Hz  
GB 0  
PC 1.00

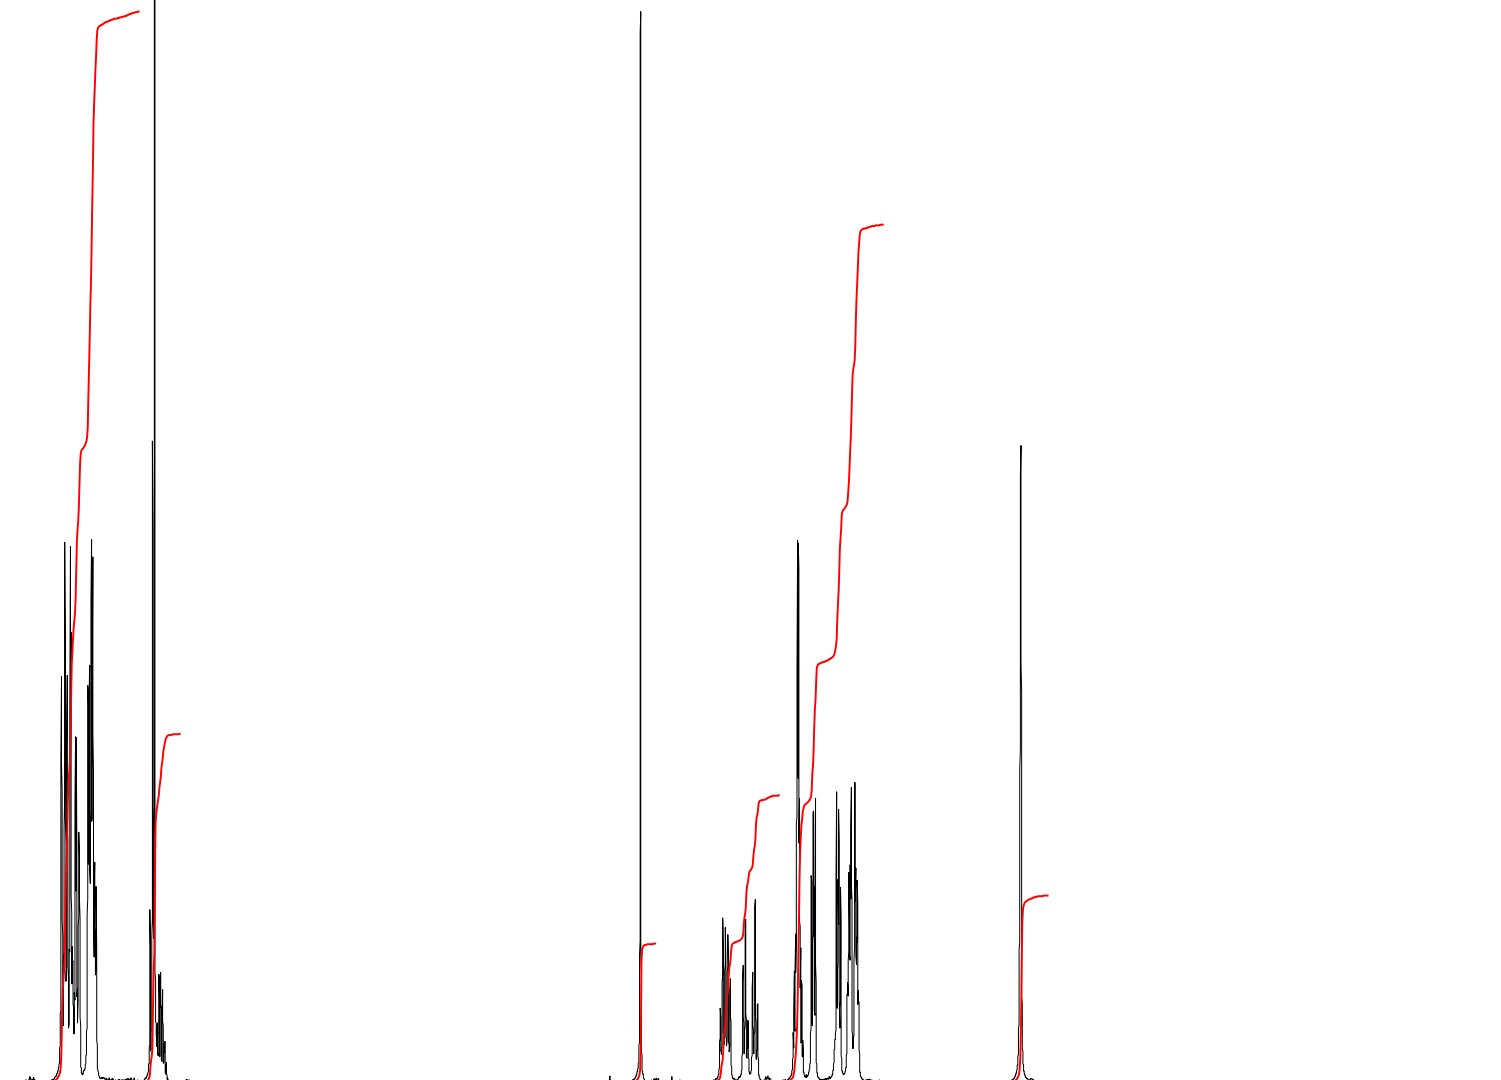

7.5 7.0 6.5 6.0 5.5 5.0 4.5 4.0 3.5 3.0 2.5 2.0 1.5 1.0 0.5 ppm

